


# COVID19

## Standardisation/Certification

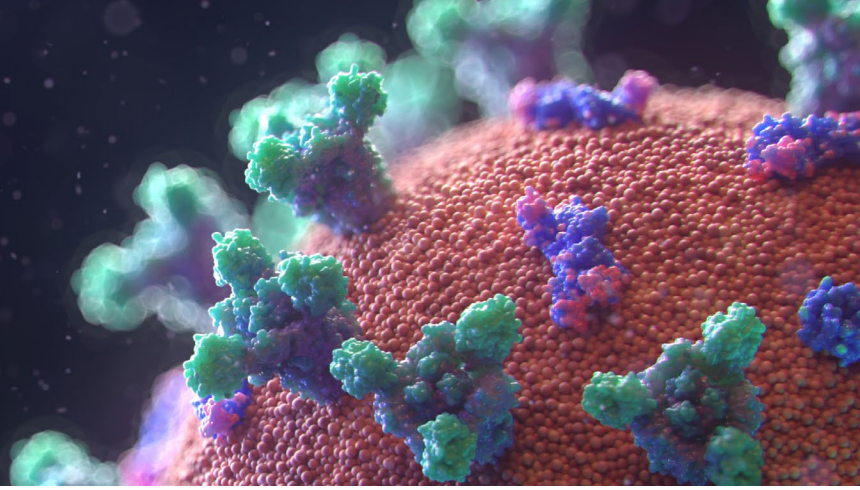

All products must have their CE marking clearly evident on the product and/or packaging and must conform to the relevant directive:

### Personal Protective Equipment Directive EU 2016/425

PPE	Standard / Certification
<b>Face Mask</b> Surgical Type IIR: face mask with loops	Must conform to: BS EN 14683:2019 or any equivalent standard Must be marked as Type IIR
<b>Respirator Masks</b> <ul style="list-style-type: none"> <li>• FFP2 &amp; FFP3</li> <li>• Single use</li> <li>• All Unvalved and Valved FFP2 and FFP3 masks</li> </ul>	Must conform to: BS EN 149:2001+A1:2009 or any equivalent standard Must be marked with the number and clearly marked valved or unvalved
<b>Helmets and hoods</b> Loose fitting type	Hoods must conform to: BS EN 12941:1998+A2:2008
<b>Protective Glasses</b>	Must conform to: BS EN 166:2002 or any equivalent standard
<b>Face Shields</b>	Must conform to: BS EN 166:2002 or any equivalent standard
<b>Protective Gowns</b> <ul style="list-style-type: none"> <li>• Sterile, non-sterile, thumb-looped</li> <li>• Must be single use</li> </ul>	BS EN 13795:2019 or equivalent standard
<b>Protective Coveralls</b> <ul style="list-style-type: none"> <li>• Must be single use</li> <li>• Performance requirements for chemical protective clothing providing protection to the full body against airborne solid particulates (type 5 clothing).</li> </ul>	All category III type 5B coveralls/protective suits must conform to: BS EN ISO 13982-1:2004+A1:2010 or any equivalent standard

[Further information and specifications for PPE can be viewed here.](#)

### PPE Supply in the South West

Edmundson Electrical have been appointed as Key Workers by the Cabinet Office to help supply Infection Control Personal Protective Equipment alongside our core business of supplying electrical products.



01803 616372